



DataVU 7 - Installation Manual

59488/1

Contents

1	Introduction	5
1.1	Preface	5
1.2	Arrangement of the documentation	6
1.3	Typographical conventions	8
2	Identifying the instrument version	9
2.1	Nameplate	9
2.2	Type designation	10
2.3	Standard accessories	11
2.4	Accessories	11
3	Installation	13
3.1	Installation site and climatic conditions	13
3.2	Mounting	13
4	Electrical connection	15
4.1	Installation notes	15
4.2	Procedure	16
4.3	Overview of the electrical isolation	17
4.4	Connection diagram	18
4.5	Connection examples concerning binary inputs/outputs	24
5	Functional test	27
6	Technical data (extract from data sheet)	29
7	Glossary	33

Contents

1.1 Preface



Please read these Operating Instructions before commissioning the instrument. Keep the manual in a place that is accessible to all users at all times.

Please assist us to improve this operating manual, where necessary.

Your comments will be appreciated.



If any difficulties should arise during commissioning, you are asked not to carry out any manipulations that could endanger your rights under the instrument warranty!

Please contact the nearest subsidiary or the head office in such a case.



When returning modules, assemblies or components, the regulations of EN 61340-5-1 and EN 61340-5-2 "Protection of electronic devices from electrostatic phenomena" must be observed. Use only the appropriate **ESD** packaging for transport.

Please note that we cannot accept any liability for damage caused by ESD.

ESD=electrostatic discharge

1 Introduction

1.2 Arrangement of the documentation

The documentation for this instrument is addressed to equipment manufacturers (OEMs) and users with appropriate technical expertise. It consists of the following parts:

Instrument documentation in printed form

59486 Operating Instructions

The operating instructions are an extract from the operating manual and cover the basic operation of the paperless recorder.

59488/59490 Installation Instructions

The installation instructions describe the installation of the recorder and the connection of the supply and signal cables. The instructions also contain a list of the technical data.

59488 Installation instructions for recorders with die-cast zinc front 59490 Installation instructions for recorders with stainless steel front

Instrument documentation in the form of PDF files

The "Instrument documentation in the form of PDF files" is on the CD that is included in the delivery.

59484 Operating Manual

It contains information about commissioning, operation, parameterization and configuration on the instrument.

59486 Operating Instructions

The operating instructions are an extract from the operating manual and cover the basic operation of the paperless recorder.

59494 Interface Description (serial interfaces)

This provides information on the communication (RS232/RS485) with supervisory systems.

Interface Description (Ethernet interface)

This provides information on the connection of a paperless recorder to a company-internal network. This description is integrated into 59494.

59496 Interface Description (PROFIBUS-DP interface)

This provides information on the connection of a paperless recorder to a PROFIBUS-DP system.

59488/59490 Installation Instructions

The installation instructions describe the installation of the recorder and the connection of the supply and signal cables. The instructions also contain a list of the technical data.

59488 Installation instructions for recorders with die-cast zinc front 59490 Installation instructions for recorders with stainless steel front

59492 Setup Program

The manual describes the function of the setup program. The setup program is available as an option.

DS-DV7-1-EN-1202

Data Sheet

The data sheet contains general information, the order details and the technical data.

59498 PC Evaluation software (PCA3000)

The operating manual describes the operation and the features of the PC evaluation software.

PCA3000 serves to visualize and evaluate process data (measurement data, batch data, messages ...). The process data can be read in via the CompactFlash memory card, or made available through the PCC software.

59500 PCA Communications software (PCC)

The operating manual describes the operation and the features of the PCA Communications software.

PCC is responsible for the data transfer from the recorder to a PC, or to a network.

1.3 Typographical conventions

Warning signs

The signs for **Danger** and **Caution** are used in this manual under the following conditions:

Danger



This symbol is used when there may be **danger to personnel** if the instructions are ignored or not followed correctly!

Caution



This symbol is used when there may be **damage to equipment or data** if the instructions are ignored or not followed correctly!

Caution



This symbol is used where special care is required when handling components liable to damage through electrostatic discharge.

Note signs

Note



This symbol is used when your **special attention** is drawn to a remark.

Reference



This symbol refers to **further information** in other manuals, chapters or sections.

Footnote

abc¹

Footnotes are remarks that **refer to specific points** in the text. Footnotes consist of two parts:

A marker in the text, and the footnote text.

The markers in the text are arranged as continuous superscript numbers.

Action instruction

·

This symbol indicates that an **action to be performed** is described.

The individual steps are marked by this asterisk, e.g.

- * Rotate control knob
- * Press control knob

2 Identifying the instrument version

2.1 Nameplate

Position The nameplate is glued onto the paperless recorder.

Contents It contains important information, such as:

Description	Designation on the nameplate	Example	
Device type	Тур	VU7-3-3-R-0-1-0	
Sales No.	VARTN	70/00xxxxxx	
Serial No.	F-Nr	0022969000008050006	
Supply voltage	₩-	110 — 240V AC +10/-15%, 48 — 63Hz	

Type Please check the type supplied against your order document. Refer to

Chapter 2.2 "Type designation" for identification of the type.

VARTN The Sales No. provides an unambiguous definition of an article from the

catalog. It is used in communication between the sales department and the

customer.

F-Nr The serial number (F-Nr.) indicates the production date (year/week). The

figures concerned are in positions 12, 13, 14, 15.


Example:

F-Nr 00229690000**0805**0006

This shows that the paperless recorder was manufactured in 2008, week 5.

2 Identifying the instrument version

2.2 Type designation

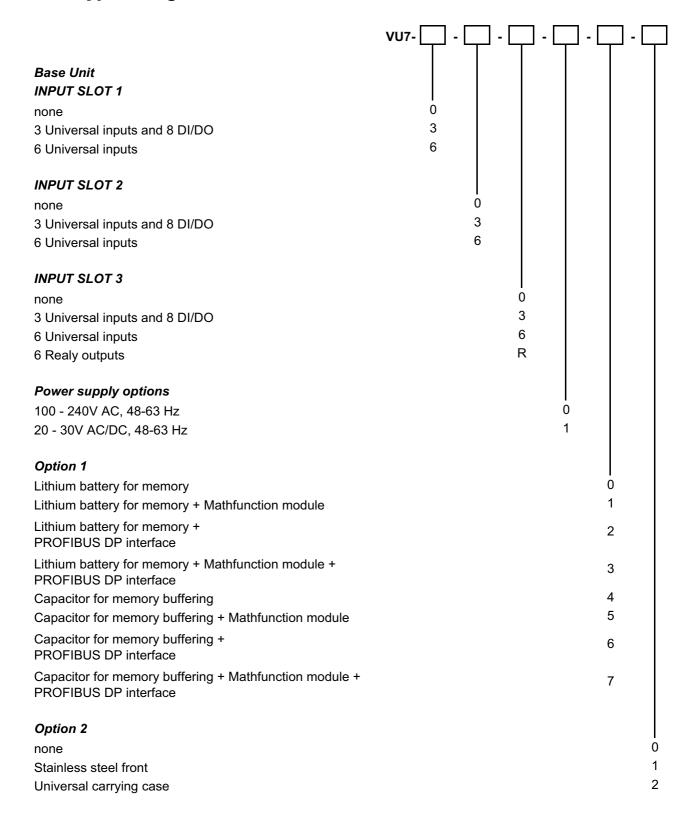

2 Identifying the instrument version

2.3 Standard accessories

- 1 Installation Instructions 59488
- 1 Operating Instructions 59486
- 4 mounting brackets
- 1 panel seal
- 1 CD with detailed operating instructions and supplementary documentation (see Chapter 1.2 "Arrangement of the documentation")

2.4 Accessories

- Setup program (incl. USB cable)
- PC Evaluation software (PCA3000)
- PCA Communications software (PCC)
- CompactFlash memory cards
- USB memory sticks
- Universal carrying case

2 Identifying the instrument version			

3.1 Installation site and climatic conditions


The installation site should be as free as possible from vibration. Electromagnetic fields, such as those caused by motors, transformers etc. should be avoided as far as possible.


The ambient temperature at the site can be 0 to 50° C, at a relative humidity of $\leq 75\%$, no condensation.

⇒ Chapter 4.1 "Installation notes"


3.2 Mounting

Views






Panel cut-out




3 Installation

Mounting in a panel

* Fit panel seal (IP65 seal).

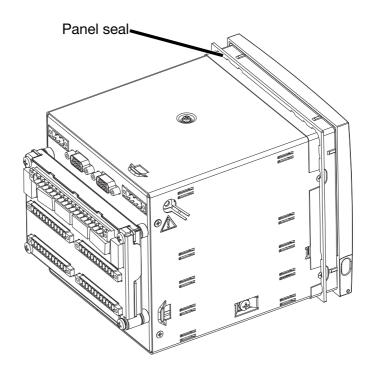

- * Insert the paperless recorder from the front into the panel cut-out.
- * From behind the panel, hook the four mounting brackets into the grooves on the sides of the housing and tighten them evenly up against the back of the panel.

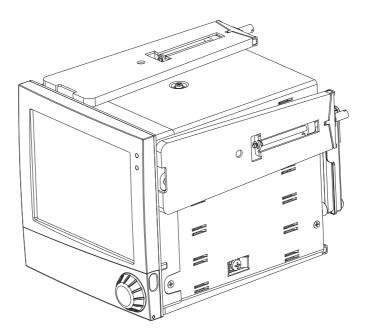

4.1 Installation notes

■ The device is designed for installation in electrical cabinets, machines, or systems. External fuse protection and shut-off must be provided for the device. The fuse must not exceed 20 A.

An instrument fuse is already built into the device itself (depending on the device design).


```
20 — 30V AC/DC, 48 — 63Hz : fuse 2.5A slow-blow 100 — 240V AC +10/-15%, 48 — 63Hz : fuse 1.25A slow-blow
```

- The choice of cable, the installation and the electrical connection must conform to the requirements of VDE 0100 "Regulations on the Installation of Power Circuits with Nominal Voltages below 1000V" or the appropriate local regulations.
- Work inside the instrument must only be carried out to the extent described and, like the electrical connection, only by qualified personnel.
- For service and repair work the device must be disconnected from the power supply (all poles).
- To generate the operating voltage of 20...30 V for Extra Low Voltage (ELV), the maximum nominal voltage of an external power supply must not exceed 240 V (line-to-line and line-to-neutral). If the external nominal voltage is greater than 240 V, an Safety Extra Low Voltage (SELV) power supply must be used. For line-to-line supply of the external power supply, the power supply must have all-pole fuse protection. The fuse must shut off both connections.
- Run input, output and supply cables separately and not parallel to one another.
- In EMC disturbed environments, all input and output cables without connection to the mains supply must be arranged as twisted and screened cables. Earth the screen on the instrument side to the earth potential.
- Ground the instrument at the PE terminal of the supply voltage connector to the protective earth conductor. This cable must have the same cross-section as that used for the supply cables. Earthing cables must be wired in a star configuration to a common earth point that is connected to the protective earth conductor of the electrical supply.
- Do not connect any additional loads to the supply terminals of the instrument.
- The device is not suitable for use in areas with an explosion hazard (Ex areas).
- Electromagnetic compatibility (EMC) conforms to the standards and regulations cited in the technical data.
 - ⇒ Chapter 6 "Technical data (extract from data sheet)"
- Inductive loads close to the instrument, such as contactors or solenoid valves, should have RC modules fitted for interference suppression.


4.2 Procedure

- * Make the electrical connection as per Chapter 4.4 "Connection diagram".
- * Apply strain relief for the connecting cables, if necessary.

Instrument variant 1

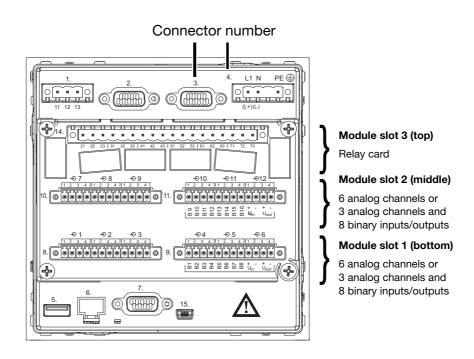


Instrument variant 2

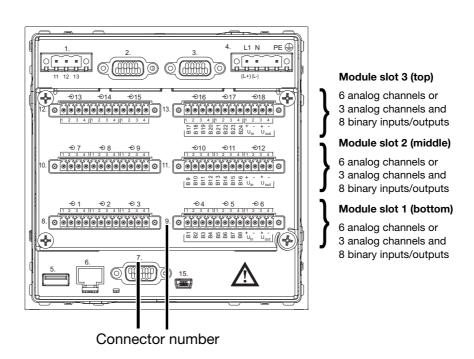

Connector summary

Connector/slot	Function
1	Relay output
2	RS232 for barcode reader
3	PROFIBUS-DP
4	Supply voltage
5	USB host interface
6	Ethernet
7	RS232 and RS485
8	Analog input
9	Analog input or binary inputs/outputs
10	Analog input
11	Analog input or binary inputs/outputs
12	Analog input
13	Analog input or binary inputs/outputs
14	Relay card (for instrument variant 1)
15	USB device interface

4.3 Overview of the electrical isolation

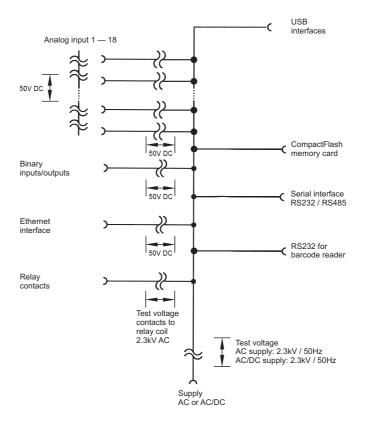

4.4 Connection diagram



The electrical connection must only be carried out by specialist personnel.

Back panel

⇒ Chapter 4.2 "Procedure"

Connections

Supply voltage

Ana	loa	inp	uts

Terminal assignment	Connector	Diagram
Supply voltage as on nameplate	Connector 4 L1 (L+) N (L-) PE	L1 N PE
Thermocouple	Connectors 8 to 11	1 2 3 4
RTD 2-wire circuit	(input 1 – 12) for instrument variant 1	1 2 3 4
RTD 3-wire circuit		1 2 3 4
RTD 4-wire circuit	** (1 2 3 4
Resistance transmitter E = end S = slider A = start	or connectors 8 to 13 (input 1 — 18)	1 2 3 4 E S A
Potentiometer in 2-wire circuit	for instrument variant 2	1 2 3 4
Potentiometer in 3-wire circuit		1 2 3 4
Potentiometer in 4-wire circuit		1 2 3 4

Analog inputs

Terminal assignment	Connector	Diagram
Voltage input 0 — 1V	Connectors 8 to 11 (input 1 – 12) for instrument	$\begin{array}{cccccccccccccccccccccccccccccccccccc$
Voltage input 0 — 10V	variant 1	$ \int_{0}^{1} \int_{0}^{2} \int_{0}^{3} \int_{0}^{4} \int_{0}^{4} U_{x} = 0 - 10V $
Current input		1 2 3 4 0 1 L 1 L 1 L 1 L 1 L 1 L 1 L 1 L 1 L 1
	or connectors 8 to 13 (input 1—18) for instrument variant 2	

Binary inputs/ outputs

Terminal assignment Connector Diagram The configuration in the instrument or in the setup program defines whether it is a binary input or binary output. B1 ... B8 Connector 9 only for modules voltage-controlled with 3 analog LOW = -3 to +5 V DCinputs HIGH = 12 to 30V DC B1 Binary input/output 1 Example: Binary input/output 2 B2 Connecting a load to **B**3 Binary input/output 3 binary output 4 (B4) В4 Binary input/output 4 and a solid-state **B**5 Binary input/output 5 relay to binary B6 Binary input/output 6 output 3 (B3) requires B7 Binary input/output 7 an external supply B8 Binary input/output 8 voltage. U_{in}+ external supply voltage Diagram of the U_{in}ground connector: U_{out}+ +24V (60mA) internal supply voltage U_{out}ground B9 ... B16 Connector 11 only for modules voltage-controlled with 3 analog Example: LOW = -3 to +5 V DCinputs Binary input 12 (B12) HIGH = 12 to 30V DC is operated from the internal supply B9 Binary input/output 9 voltage. B10 Binary input/output 10 Binary input/output 11 B11 B12 Binary input/output 12 Diagram of the B13 Binary input/output 13 connector: Binary input/output 14 B14 Binary input/output 15 B15 89 810 811 812 813 814 816 Uin+ Binary input/output 16 1 2 3 4 1 2 3 4 1 B16 U_{in}+ external supply voltage U_{in}ground U_{out}+ +24V (60mA) internal supply voltage U_{out}ground

	Terminal assignment	Connector	Diagram
Binärein-/ -ausgänge	voltage-controlled LOW = -3 to +5 V DC HIGH = 12 to 30 V DC B17 Binary input/output 17 B18 Binary input/output 18 B19 Binary input/output 19 B20 Binary input/output 20 B21 Binary input/output 21 B22 Binary input/output 21 B22 Binary input/output 22 B23 Binary input/output 23 B24 Binary input/output 23 B24 Binary input/output 24 Uin+ external supply voltage Uin- ground Uout+ +24 V (60 mA) internal supply voltage Uout- ground	Connector 13 only for instrument variant 2 and on modules with 3 analog inputs	Example: Binary input 20 (B20) is operated from the internal supply voltage. Diagram of the connector: Light Street Str
Relay outputs	Relay 1 - alarm changeover (SPDT)	Connector 1	12 11 13
	Relay 2 changeover (SPDT)	Connector 14 only for	22 21 23
	Relay 3 changeover (SPDT)	instrument variant 1	32 31 33
	Relay 4 changeover (SPDT)		42 41 43
	Relay 5 changeover (SPDT)		52 51 53
	Relay 6 changeover (SPDT)		62 61 63
	Relay 7 changeover (SPDT)		72 71 73


Interfaces

Terminal assignment	Connector	Diagram
RS232C for barcode reader 9-pin SUB-D socket connector 2 RxD receive data 3 TxD transmit data 5 GND ground	Connector 2	6789
PROFIBUS-DP 9-pin SUB-D socket connector (extra code)	Connector 3	6789
 3 RxD/TxD-P B conductor Receive/transmit data positive 5 DGND Data transmission ground 6 VP supply voltage positive 8 RxD/TxD-N A conductor Receive/transmit data negative 		
USB host interface for memory sticks	Connector 5	
The recorder without stainless steel front also has a USB host interface on the front panel, connected in parallel. The two interfaces cannot both be operated at the same time.		
Ethernet RJ45 socket connector	Connector 6	
1 TX+ transmit data + 2 TX- transmit data - 3 RX+ receive data + 6 RX+ receive data -		اتبي-
RS232C 9-pin SUB-D socket connector	Connector 7	5 4 3 2 1
(switchable to RS485)		9876
2 RxD receive data 3 TxD transmit data 5 GND ground		


Terminal assignment	Connector	Diagram
RS485 9-pin SUB-D socket connector (switchable to RS232) 3 TxD+/RxD+ Transmit/receive data + 5 GND ground 8 TxD-/RxD- Transmit/receive data -	Connector 7	5 4 3 2 1
USB device interface for connecting a PC The recorder without stainless steel front also has a USB device interface on the front panel, connected in parallel. The two interfaces cannot both be operated at the same time.	Connector 15	

4.5 Connection examples concerning binary inputs/outputs


Binary inputs Triggering via external relays and external supply voltage:

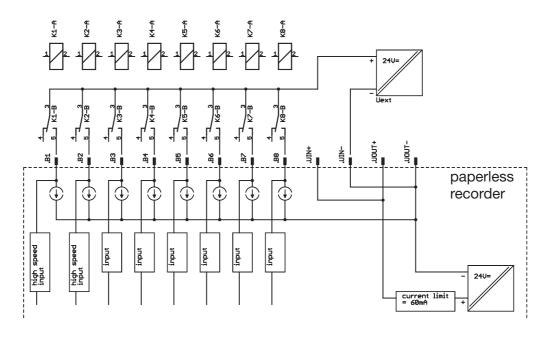


Triggering via external relays and internal supply voltage:

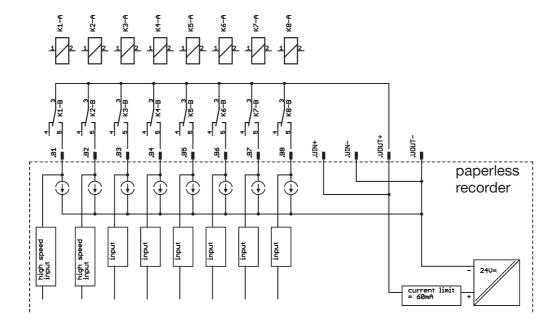

Triggering via external opto-coupler and internal supply voltage:

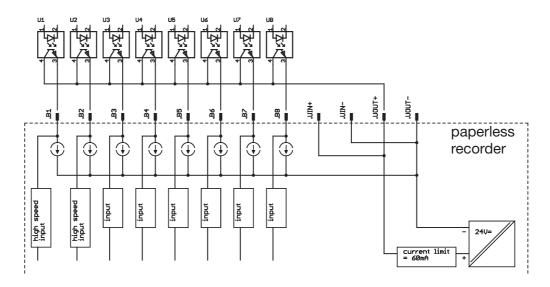


Triggering via external switches (potential-free) and internal supply voltage:

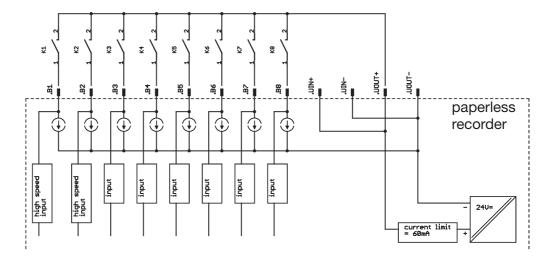


Binary outputs

Triggering of external relays via external supply voltage:

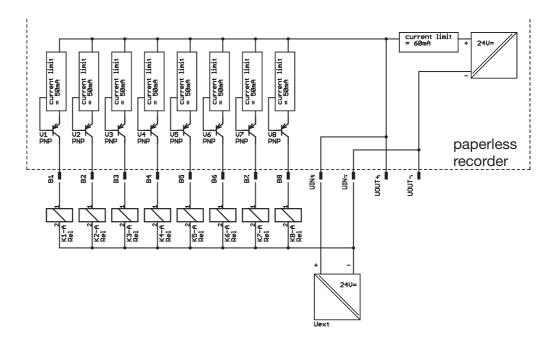

Triggering of external relays via internal supply voltage:

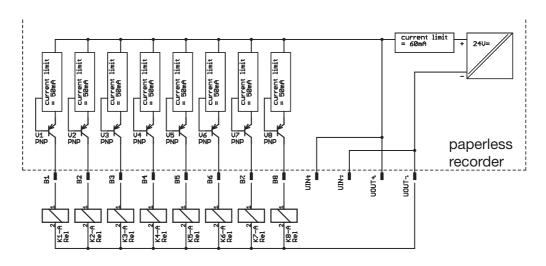




By triggering the external relays via the internal supply voltage the total current must not exceed 60 mA.

After the paperless recorder has been installed and wired up, it can be commissioned. After applying or switching on the supply voltage, the start-up screen will appear for a short time.

The visualization will start automatically after the initialization phase.

Visualization

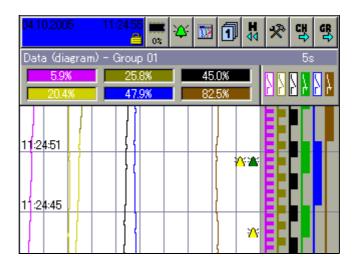

The paperless recorder is now in the recording phase.

Further steps



The recorder can be configured by an authorized person, either by using the control knob (rotating and pressing) or with the help of the PC setup program.

Further information about configuration can be found in the Operating Manual 59484.

Finally, make another check that the connection, configuration and function of the recorder are all correct.

_	— .		_1:	!		1 4	est
.		ın	CT		na	I T	esi

Analog inputs

Thermocouple

Designation	Туре	Standard	Meas. range	Accuracy ¹	
Fe-CuNi	L	DIN 43 710	-200 to +900°C	±0.1%	
Fe-CuNi	J	EN 60 584	-200 to +1200°C	±0.1% from -100°C	
Cu-CuNi	U	DIN 43 710	-200 to +600°C	±0.1% from -150°C	
Cu-CuNi	Т	EN 60 584	-270 to +400°C	±0.1% from -150°C	
NiCr-Ni	K	EN 60 584	-200 to +1372°C	±0.1% from -80°C	
NiCr-CuNi	E	EN 60 584	-200 to +1000°C	±0.1 % from -80°C	
NiCrSi-NiSi	N	EN 60 584	-100 to +1300°C	±0.1% from -80°C	
Pt10Rh-Pt	S	EN 60 584	0 to 1768°C	±0.15%	
Pt13Rh-Pt	R	EN 60 584	0 to 1768°C	±0.15%	
Pt30Rh-Pt6Rh		EN 60 584	0 to 1820°C	±0.15% from 400°C	
W3Re/W25Re			0 to 2495°C	±0.15% from 500°C	
W5Re/W26Re	С		0 to 2320°C	±0.15% from 500°C	
W3Re/W26Re			0 to 2400°C	±0.15% from 500°C	
Chromel-copel		GOST R 8.585-2001	-200 to +800°C	±0.15% from -80°C	
Chromel-alume		GOST R 8.585-2001	-200 to +1372°C	±0.1% from -80°C	
PLII (Platinel II)			0 to 1395°C	±0.15%	
Shortest span			· · · · · · · · · · · · · · · · · · ·	hromel-alumel, PLII: 100°C /26Re, chromel-copel: 500°C	
Range start/en	d		freely programmable with	in the limits, in 0.1°C steps	
Cold junction			Pt100 internal or thermostat external constant		
Cold junction a	ccurac	y (internal)	± 1°C		
Cold junction to	empera	ature (external)	-50 to +150°C adjustable		
Sampling cycle			Channel 1 - 18: 125ms in total		
Input filter			2nd order digital filter; filter constant adjustable from 0 to 10.0 sec		
Electrical isolation			see "Electrical data" on page 5 and		
			"Overview of the electrical isolation" on page 16		
Resolution			>14 bit		
Features			also progra	mmable in °F	

¹ The linearization accuracy refers to the maximum measuring range. The linearization accuracy is reduced with short spans.

Resistance thermometer

Designation	Standard	Connection circuit	Meas. range	Accuracy ¹	Meas. curr.
Pt100	EN 60 751 (TC = 3.85*10 ⁻³ 1/°C)	2/3-wire 2/3-wire 4-wire	-200 to +100°C -200 to +850°C -200 to +850°C	±0.5°C ±0.8°C ±0.5°C	≈ 250µA ≈ 250µA ≈ 250µA
Pt100	JIS 1604 (TC = 3.917*10 ⁻³ 1/°C)	2/3-wire 2/3-wire 4-wire	-200 to +100°C -200 to +650°C -200 to +650°C	±0.5°C ±0.8°C ±0.5°C	≈ 250 μA ≈ 250 μA ≈ 250 μA
Pt100	GOST 6651-94 A.1 (TC = 3.91*10 ⁻³ 1/°C)	2/3-wire, 4-wire 2/3-wire, 4-wire	-200 to +100°C -200 to +850°C	±0.5°C ±0.8°C	≈ 250µA ≈ 250µA
Pt500	EN 60 751 (TC = 3.85*10 ⁻³ 1/°C)	2/3-wire, 4-wire 2/3-wire, 4-wire	-200 to +100°C -200 to +850°C	±0.5°C ±0.9°C	≈ 100µA ≈ 100µA
Pt1000	EN 60 751 (TC = 3.85*10 ⁻³ 1/°C)	2/3-wire 2/3-wire 4-wire	-200 to +100°C -200 to +850°C -200 to +850°C	±0.5°C ±0.8°C ±0.5°C	≈ 100 μA ≈ 100 μA ≈ 100 μA
Ni 100	DIN 43 760 (TC = 6.18*10 ⁻³ 1/°C)	2/3-wire, 4-wire	-60 to +180°C	±0.4°C	≈ 250µA
Pt50	ST RGW 1057 1985 (TC = 3.91*10 ⁻³ 1/°C)	2/3-wire 2/3-wire 4-wire 4-wire	-200 to +100°C -200 to +1100°C -200 to +100°C -200 to +1100°C	±0.5°C ±0.9°C ±0.5°C ±0.6°C	≈ 250 µA ≈ 250 µA ≈ 250 µA ≈ 250 µA
Cu 50	(TC = 4.26*10 ⁻³ 1/°C)	2/3-wire 2/3-wire 4-wire 4-wire	-50 to +100°C -50 to +200°C -50 to +100°C -50 to +200°C	±0.5°C ±0.9°C ±0.5°C ±0.7°C	≈ 250 µA ≈ 250 µA ≈ 250 µA ≈ 250 µA

Designation	Standard	Connection circuit	Meas. range	Accuracy ¹	Meas. curr.	
Cu 100	GOST 6651-94 A.4 (TC = 4.26*10 ⁻³ 1/°C)	2/3-wire 2/3-wire 4-wire 4-wire	-50 to +100°C -50 to +200°C -50 to +100°C -50 to +200°C	±0.5°C ±0.9°C ±0.5°C ±0.6°C	≈ 250 µA ≈ 250 µA ≈ 250 µA ≈ 250 µA	
Connection cir	rcuit		2-, 3-, or 4-	wire circuit		
Shortest span		15°C				
Sensor lead resistance		max. 30 per conductor for 3-wire/4-wire circuit max. 10 per conductor for 2-wire circuit				
Range start/end		fro	freely programmable within the limits, in 0.1 °C steps			
Sampling cycle		Channel 1 - 18: 125ms in total				
Input filter	Input filter		2nd order digital filter; filter constant adjustable from 0 to 10 sec			
Electrical isolation		see "Electrical data" on page 5 and "Overview of the electrical isolation" on page 16				
Resolution	Resolution		>14 bit			
Features		also programmable in °F				

¹ The linearization accuracy refers to the maximum measuring range. The linearization accuracy is reduced with short spans.

Resistance transmitter and potentiometer

Designation	Meas. range	Accuracy ¹	Meas. curr.
Resistance transmitter	up to 4000Ω	±4Ω	≈ 100 µA
Potentiometer	< 400 Ω	±400mΩ	≈ 250 µA
	$\geq 400\Omega$ to 4000Ω	±4Ω	≈ 100µA
Connection circuit		resistance transmitter:	
		potentiometer: 2-/3-/4	1-wire circuit
Shortest span		60Ω	
Sensor lead resistance		max. 30 per conductor fe	or 4-wire circuit
	r	max. 10 per conductor for	r 2-/3-wire circuit
Resistance values	free	ly programmable within th	e limits, in 0.1 steps
Sampling cycle		Channel 1 - 18: 125	ms in total
Input filter	2nd order di	gital filter; filter constant a	djustable from 0 to 10.0 sec
Electrical isolation		see "Electrical data" or	n page 5 and
	"O	verview of the electrical is	olation" on page 16
Resolution		>14 bit	

¹ The linearization accuracy refers to the maximum measuring range. The linearization accuracy is reduced with short spans.

Basic range	Accuracy ¹	Input resistance		
-12 to +112mV	±100μV	R _E ≥1 MΩ		
-10 to +210mV	±240μV	$R_{E} \ge 470 \text{ k}\Omega$		
-1.5 to +11.5V	±6mV	R _E ≥ 470 kΩ		
-0.12 to +1.12V	±1 mV	$R_E \ge 470 \text{ k}\Omega$		
-1.2 to +1.2V	±2mV	$R_E \ge 470 \text{ k}\Omega$		
-11.2 to +11.2V	±12mV	R _E ≥ 470 kΩ		
Shortest span		5mV		
Range start/end	freely pro	grammable within the limits in 0.01 mV steps		
-1.3 to +22mA	±20μA	burden voltage ≤ 3 V		
-22 to +22 mA	±44μA	burden voltage ≤ 3V		
Shortest span		0.5 mA		
Range start/end	freely prog	freely programmable within the limits in 0.01 mA steps		
Overrange/underrange		according to NAMUR NE 43		
Sampling cycle		Channel 1 - 18: 125ms in total		
Input filter	2nd order digita	2nd order digital filter; filter constant adjustable from 0 to 10.0 sec		
Electrical isolation	:	see "Electrical data" on page 5 and		
		iew of the electrical isolation" on page 16		
Resolution		>14 bit		

¹ The linearization accuracy refers to the maximum measuring range. The linearization accuracy is reduced with short spans.

Transducer short circuit/break

	Short-circuit ¹	Break ¹
Thermocouple	not detected	detected
Resistance thermometer	detected	detected
Resistance transmitter	not detected	detected
Potentiometer	not detected	detected
Voltage ≤ ± 210mV	not detected	detected
Voltage > ± 210 mV	not detected	not detected
Current	not detected	not detected

¹ Programmable reaction of device, e.g. triggering alarm

Binary inputs/outputs (option)

Input or output	configurable as input or output
Number	8, 16 or 24, depending on the device version,
	to DIN VDE 0411, Part 500; max. 25Hz, max. 32V
Input	
- level	logic "0": -3 to +5V (input current max. ±1 mA),
	logic "1": 12 to 30V ($2.5 \text{mA} \le \text{input current} \le 5 \text{mA}$)
 counting frequency 	8Hz
High-speed input	the first two binary inputs of each module (B1, B2, B9, B10, B17, B18),
	if the module is not fitted with relays or 6 analog inputs
- task	count function, e.g. for flow measurement
 counting frequency 	10kHz
Output	
- type	open-collector output, switches relative to positive voltage
- level	logic "0": transistor is inhibited
	(max. permissible voltage across switching transistor 30V, max. leakage current 0.1 mA)
	logic "1": transistor is switched on
	(max. voltage across switching transistor 1.6V, max. current 50 mA)
- sampling cycle	at least 1sec (1Hz)

Outputs

1 relay (ex-factory)	changeover (SPDT), 3A, 230V AC ¹
6 relays (option)	changeover (SPDT), 3A, 230V AC ^{1,2}

With resistive load. ² It is not permissible to mix SELV circuits and supply circuits.

Interfaces

D0000/D0405 (7)	Oh. 1 aviitababla bahvaan D0000 and D0405
RS232/RS485 (connector 7)	Qty. 1, switchable between RS232 and RS485
- protocol	Modbus master, Modbus slave and barcode reader
- baud rate	9600, 19200, 38400
- modem	can be connected
- connector	SUB-D
- external inputs	via the Modbus master/slave function, 24 analog and 24 binary
RS232 for barcode reader (connector 2)	Qty. 1
- protocol	Modbus master, Modbus slave and barcode reader
- baud rate	9600, 19200, 38400
- connector	SUB-D
- external inputs	via the Modbus master/slave function, 24 analog and 24 binary
Ethernet (connector 6)	
- quantity	max. 1
- protocols	TCP, IP, HTTP, DHCP, SMTP, ModbusTCP
- baud rate	10Mbits/sec, 100Mbits/sec
- connector	RJ45
- data format	HTML
USB host (connector 5)	
- quantity	2 (or 1 with stainless steel front),
	connector 5 and front connector (not with stainless steel front); no parallel operation
- use	for connecting a memory stick
- max. current	100mA
USB device (connector 15)	
- quantity	2 (or 1 with stainless steel front),
•	connector 15 and front connector (not with stainless steel front); no parallel operation)
- use	for connecting to the (master) computer

Screen

Resolution / size	320 x 240 pixels / 5.5"
Type / number of colors	TFT color screen / 256 colors
Screen refresh rate	> 150Hz
Brightness setting	adjustable on instrument
Screen saver (switch-off)	through waiting time or control signal

Electrical data

Supply voltage (switch-mode PSU)	100 - 240V AC +10/-15%, 48 - 63Hz or 20 - 30V AC/DC, 48 - 63Hz (ELV)
Electrical safety	to EN 61 010, Part 1, August 2002
	overvoltage category II, pollution degree 2
Protection class I	terminal for PE conductor
Test voltages (type test)	
- mains supply circuit to meas. circuit	with AC supply: 2.3kV/50Hz, 1min,
	with AC/DC supply: 2.3 kV/50Hz, 1 min
- mains supply circuit to housing	with AC supply: 2.3kV/50Hz, 1min,
(protective conductor)	with AC/DC supply: 2.3kV/50Hz, 1 min
- measuring current circuits to	
meas. current circuit and housing	500V/50Hz, 1min
- electrical isolation	
between analog inputs	up to 30V AC and 50V DC
Supply voltage error	< 0.1% of range span
Power consumption	approx. 40VA
Data backup	CompactFlash memory card
Electrical connection	
- mains supply and relays	at rear through pluggable screw terminals, 5.08mm raster,
·	max. conductor cross-section ≤ 2.5 mm ² or 2x 1.5 mm ² with ferrules
- analog and binary inputs	at rear through pluggable screw terminals, 3.81 mm raster,
	max. conductor cross-section ≤ 1.5mm ²

Environmental influences

Ambient temperature range	0 to +50°C	
Ambient temperature effect	0.03%/°C	
Storage temperature range	-20 to +60°C	
Climatic conditions	≤75% relative humidity, no condensation	
EMC	EN 61 326-1	
- interference emission	Class A - only for industrial use -	
- immunity to interference	to industrial requirements	

Housing

Housing front	zinc die-casting, optionally in stainless steel (extra code)			
Housing type	housing for flush-panel mounting to IEC 61 554, in stainless steel			
Bezel size	144mm x 144mm to IEC 61 554			
Depth behind panel	193mm (incl. terminals)			
Panel cut-out	138 ^{+1.0} mm x 138 ^{+1.0} mm to IEC 61 554			
Panel thickness	2 - 40mm			
Housing mounting	in panel to DIN 43 834			
Operating position	unrestricted, but taking into account the viewing angle of the screen, horizontally ±65°, vertically +40° to -65°			
Enclosure protection	to EN 60 529 Category 2, front IP65, rear IP20			
Weight	approx. 3.5kg			

Α

Accessories 11

В

Back panel 18

C

Climatic conditions 13 Commissioning 5 CompactFlash 7 Connection diagram 18

D

Documentation, arrangement of 6

E

Electrical connection 15 Electrostatic discharge (ESD) 5

F

Functional test 27

I

Installation 13
Installation notes 15
Installation site 13
Instrument documentation in printed form 6
Instrument documentation in the form of PDF files 6
Instrument version, identification of 9
Introduction 5

M

Mounting 13

N

Note signs 8

P

Panel mounting 14

R

Returning 5

S

Standard accessories 11

T

Technical data 29
Type designation 10
Typographical conventions 8

V

Views 13 Visualization level 27

W

Warning signs 8 Warranty 5

2009-12-11/00578763



Austria T: +43 (0) 2236 691 121
China T: +86 22 8398 8098
France T: +33 (1) 77 80 90 40
Germany T: +49 (0) 561 505 1307
UK T: +44 (0) 1273 606 271
USA T: +1 800 866 6659

Email Inquiries@West-CS.com
Website www.West-CS.com



